

# Ling-6(HL) Scoring Sheet

---


Name: \_\_\_\_\_ D.O.B: \_\_\_\_\_

Date: \_\_\_\_\_ Respondent: \_\_\_\_\_

Notes on testing conditions: \_\_\_\_\_

- Test method:       Standard     CPA       VRA
- Reliability:       Good       Fair       Poor
- Test type:         Aided       Unaided     CI     Bone conducted     BAHA
- Masking (unaided ear)?     n/a       Yes       No

Plot the corrected threshold values in dB HL below:

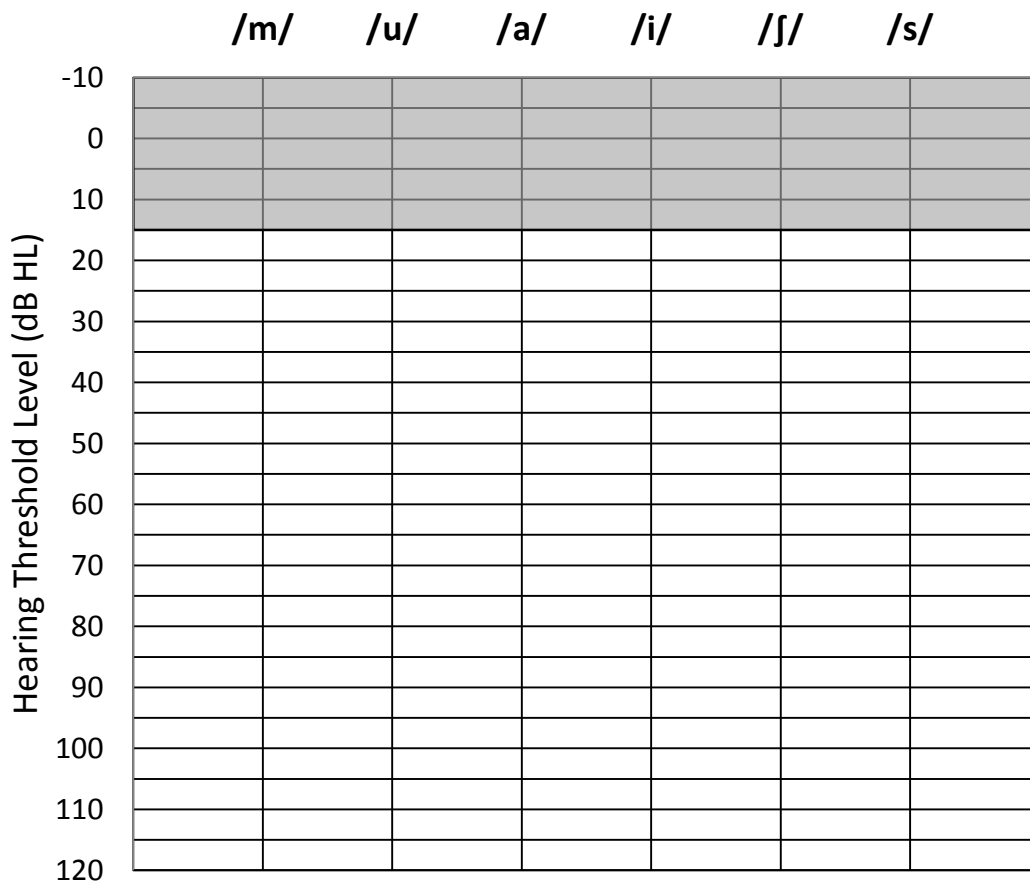

Grey region shows the normal hearing range. Values assume binaural sound field testing at zero degrees azimuth.